



FICHA TÉCNICA DE PRODUTO

PRODUCT DATASHEET

HMI – Automação e Instrumentação, Lda.

Travessa da Indústria, nº 111
4780-573 Santo Tirso
PORTUGAL

Tel. +351 252 850 501
Fax. +351 300 013 487


Web: www.hmi.pt

Email: hmi@hmi.pt

ABB MEASUREMENT & ANALYTICS | DATA SHEET | DS/ADS550-EN REV. I

Navigator 500

Dissolved oxygen analyzer

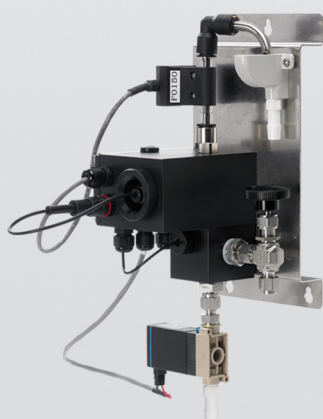

Measurement made easy

Accurate and reliable measurement of dissolved oxygen in high-purity water

Monitors both low and high dissolved oxygen concentrations

- Suitable for measurement during two-shifting and baseload operations on power stations

Automatic calibration

- Minimizes manual intervention and protects sensor during calibration

Fast response

- Reacts quickly to rapid changes in plant conditions

Thermal protection

- Protects sensor in the event of cooling water failure

Disposable sensor

- Minimizes downtime and avoids the need for skilled personnel to carry out sensor refurbishment

Comprehensive diagnostics

- Provides sensor condition and analyzer status data

Connect multiple wet sections to a single transmitter

- Reduces footprint and installation costs

The Navigator 500 range

The Navigator 500 range of analyzers from ABB are designed for high-purity water treatment applications and power cycle chemistry monitoring.

The analysis and signal conditioning is conducted within the Navigator 550's advanced wet section that houses the sensing technology. The accurate measurement result is transmitted digitally to the Navigator 540 transmitter.

The Navigator 540 universal transmitter enables connection of up to four different Navigator 550 wet sections, and is available with optional features such as SD™ card data retrieval and graphical trending, as well as additional outputs and communication options.

The following parameters are available in the Navigator 500 range:

Navigator 500

- Dissolved oxygen
- Sodium
- Hydrazine

Navigator 500 dissolved oxygen analyzer

The Navigator 500 dissolved oxygen analyzer provides continuous monitoring and control of power station boiler feed water/steam condensate.

The wet-section houses ABB's maintenance-free electrochemical cell that accurately measures the amount of dissolved oxygen in the water.

Measurement results are updated digitally to the Navigator 540 transmitter where process trends of up to four separate wet sections can be viewed locally on the color display. Users of this system also benefit from the analyzer's low maintenance requirements, ease-of-use, auto-calibration and proven sensing performance.

Process data, together with the content of alarm and audit logs within the transmitter, can be saved to a removable media for record keeping and analysis using ABB's DataManager Pro data analysis software.

Navigator 500 transmitter



Sodium
Hydrazine
Dissolved oxygen


Navigator wet sections



Sodium



Hydrazine



Dissolved oxygen
(ADS550)



Dissolved oxygen
(ADS551)

Figure 1 Navigator 500 family

Applications

Typical applications for the Navigator 500 dissolved oxygen analyzer include:

- Protection against corrosion caused by excessive dissolved oxygen concentrations
- De-aerator efficiency indication
- Hydrazine dosing efficiency indication

Low-level dissolved oxygen on boiler plant

The need for accurate monitoring

Accurate measurement of dissolved oxygen is essential for efficient, cost-effective operation of boiler plant. In its dissolved form, oxygen is highly corrosive to most metals, especially the mild steel used for boiler tubes. The presence of even small quantities of dissolved oxygen in boiler water can severely impair a boiler's operation, causing corrosion of its vital components and significantly reducing its working life.

To minimize damage caused by corrosion, it is therefore necessary to reduce dissolved oxygen to the lowest possible level, typically in the order of seven parts per billion or less. In some applications, particularly those operating once-through boilers, it is preferable to add oxygen to the boiler feedwater, causing a layer of soft hematite to form on the boiler tubes. Hydrazine is then added that reacts with the hematite, converting it to a hard layer of magnetite that protects the tubes from further corrosion.

Monitoring should be carried out wherever there is a risk of oxygen ingress into the boiler feedwater. An effective system monitors dissolved oxygen at key points including the extraction pump discharge, the de-aerator inlet and outlet, and the economizer or boiler inlet.

The Navigator 500 solution

The significant variations in oxygen levels during the load cycle of a plant, combined with the different levels required for different boiler chemistry regimes, require an analyzer that offers a fast response across both high- and low-level dissolved oxygen concentrations.

The Navigator 500 dissolved oxygen analyzer uses a galvanic-type sensor to accurately measure dissolved oxygen levels in process feedwater. Accurate and reliable, it requires no maintenance, and can measure dissolved oxygen concentrations up to 20 ppm.


Featuring a separate wet section and transmitter, the Navigator 500 dissolved oxygen analyzer gives users the option of adding up to four wet sections to one transmitter, enabling measurement of samples from different points in the boiler feedwater line. This feature also allows users to mix and match different sensor types from the Navigator 550 range of hydrazine and sodium wet sections.

Overview of Navigator 500 dissolved oxygen analyzer



Transmitter

- Simple navigation and easy-to-use menu system
- Full audit trail logs
- SD card or USB archiving
- Graphical trending
- Password-protected security
- Connect up to four wet sections in the Navigator 500 range

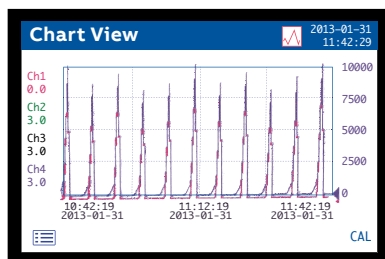


Graphical trending

- Measurement trends of each connected wet section can be easily and clearly viewed locally on the graphical color display


No.	Event	Date	Time
01	Power Failure	2013-01-31	11:14:18
02	Power Recovery	2013-01-31	09:29:39
03	Power Failure	2013-01-23	12:30:29
04	Power Recovery	2013-01-21	12:29:44

Full audit trail logs

- Diagnostic messages, alarm events, calibration details and system activity are stored in the transmitter audit logs for review

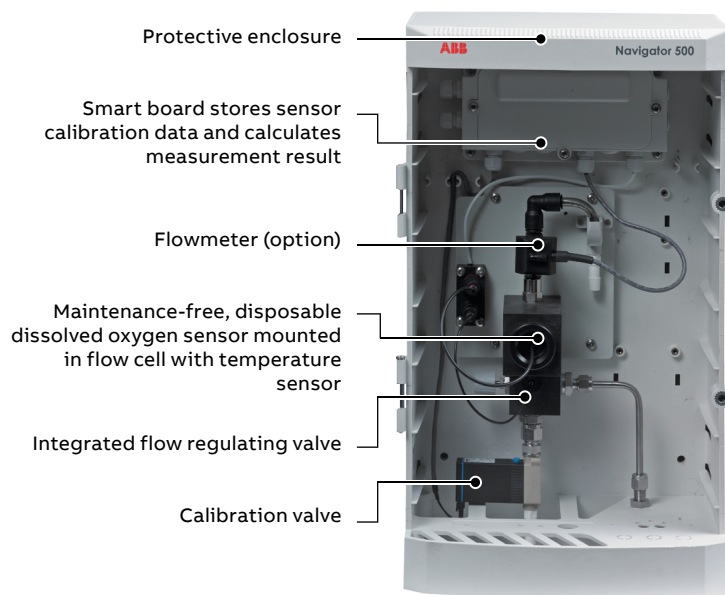

ADS550 wet section

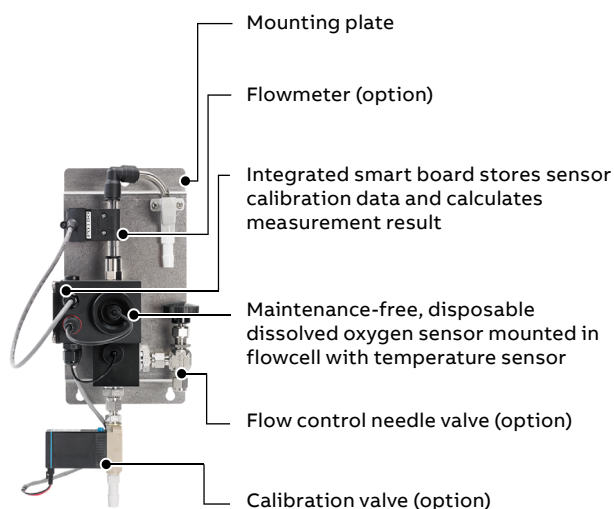

ADS551 wet section

Accurate and reliable measurement

The Navigator 500 dissolved oxygen analyzer has been designed for ease-of-use and maintenance simplicity, while offering the benefits of flexible communication and advanced data acquisition.

Measuring principle

The Navigator 500 dissolved oxygen analyzer uses a disposable galvanic cell in a custom-designed flow cell. Sample flow is adjusted easily by a flow regulating needle valve and monitored by an optional flowmeter. A temperature sensor fitted in the flowcell, measures the temperature of the sample.

The signal from the dissolved oxygen sensor and the temperature sensor is passed to the smart board located within the Navigator 550 wet section. The smart board accurately calculates the dissolved oxygen measurement result and transfers it digitally to the Navigator 540 transmitter.

Maintenance-free disposable sensor


ABB dissolved oxygen sensors are maintenance-free and long lasting. Their encapsulated design removes the requirement for time-consuming maintenance such as membrane changes or electrolyte replenishment. The easy replacement procedure for the maintenance-free DO sensor just takes seconds, saving further valuable time and cost.




Figure 2 Easy sensor replacement

Simple automatic calibration


The Navigator 500 dissolved oxygen analyzer features automatic calibration that verifies the analyzer's performance and calculates sensor efficiency. During calibration the sample is diverted, exposing the dissolved oxygen sensor to air.

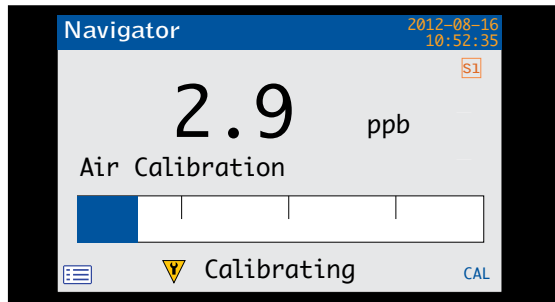


Once the calibration routine is complete, sensor efficiency is calculated and displayed, providing the user with a valuable indication of sensor life.

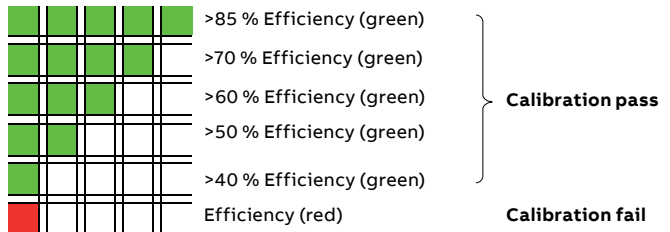

The frequency of automatic calibration can be scheduled by the user to occur from daily to bi-monthly intervals. Calibration can also be initiated manually by the operator.

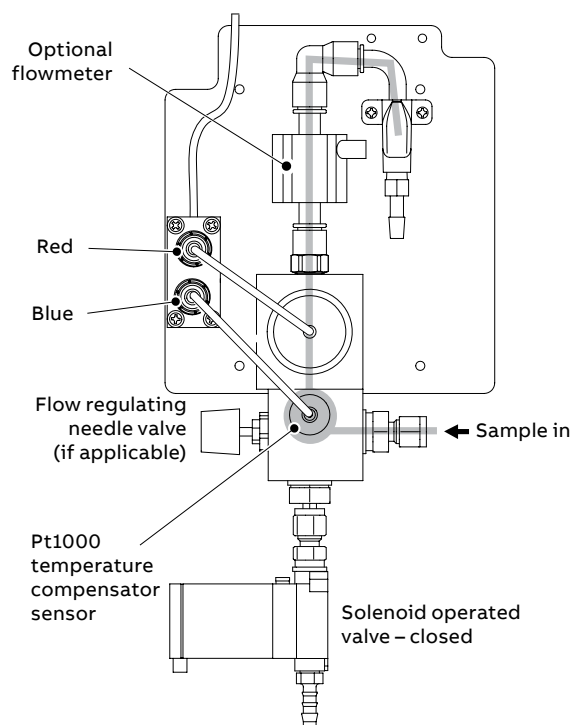

Flow during normal operation

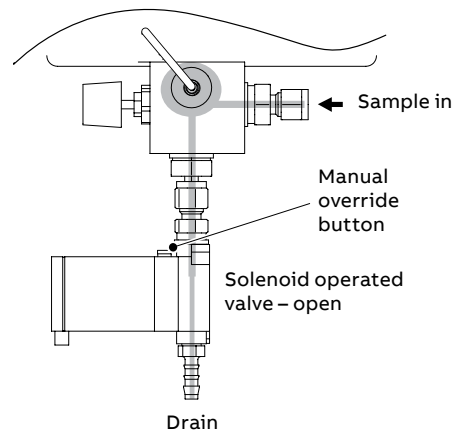

Flow during calibration or thermal overload condition

Figure 3 Flow conditions

Specifications – System

Operation

Measuring range

0 to 20,000 ppb

Units of measure

ppb, µg/L, µg/kg

Accuracy

±5 % of reading or ±1 ppb, whichever is the greater

Repeatability

±3 % of reading or ±1 ppb, whichever is the greater

Response time

1 minute for a 90 % step change

Resolution

0.1 ppb

Temperature compensation

5 to 55 °C (41 to 131 °F) automatic using a Pt1000

Salinity correction

Preset within the range 0 to 80 ppt

Barometric pressure correction

Preset within the range 500 to 800 mmHg

AutoCal frequency

Programmable from 1 to 7 days or 1 to 8 weeks

Sample temperature

5 to 55 °C (41 to 131 °F)

Sample pressure

2 bar gauge (29 psi) maximum

Sample flow rate

100 to 300 mL/min

Sample connections

¼ in or 6 mm OD pipe (stainless steel recommended)

Environmental data

Ambient operating temperature:

0 to 55 °C (32 to 131 °F)

Ambient operating humidity:

Up to 95 % RH non-condensing

Storage temperature:

-20 to 70 °C (-4 to 158 °F) without sensor

0 to 55 °C (32 to 131 °F) with sensor

Approvals, certification and safety

Safety approval

cULus

CE mark

Covers EMC & LV Directives

(including latest version EN 61010)

General safety

EN61010-1

Pollution category 2

Insulation category 2

EMC

Emissions & immunity

Meets requirements of IEC61326 for an industrial environment and domestic emissions

Maintenance

Periodic calibration:

User-defined

Specifications – Wet section

Mechanical data

Protection

IP54

Dimensions – ADS550

Height: 480 mm (18.90 in)

Width: 290 mm (11.41 in) – door shut

Depth: 185 mm (7.28 in) door closed – min.

(excluding fixing brackets)

Weight: 4.5 kg (10 lb)

Dimensions – ADS551

Height: 194 mm (7.64 in) minimum – excluding glands

Width: 214 mm (8.42 in) – excluding glands

Depth: 98 mm (3.85 in) door closed; min. – excluding fixing brackets

Weight: 1.5 kg (3.3 lb)

Electrical

Power supply ranges (supplied by transmitter)

24 V DC max.

Power consumption

8 W max.

Specifications – Transmitter

Operation

Display

89 mm (3.5 in) color ¼ VGA TFT, liquid crystal display (LCD) with built-in backlight and brightness/contrast adjustment

Language

English, German, French, Italian, Spanish

Keypad

6 tactile membrane keys:

Group select/left cursor, view select/right cursor, menu key, up, down, enter key

No of inputs

Up to 4 single-stream or 1 multistream wet section

Mechanical data

Protection

IP66/NEMA 4X

Dimensions

Height:

194 mm (7.64 in) min. (excluding glands)

Width:

214 mm (8.42 in) – excluding glands

Depth:

98 mm (3.85 in) door closed – min. (excluding fixing brackets)

Weight:

1.5 kg (3.3 lb)

Materials of construction

Glass-filled polycarbonate

Security

Password protection

Calibrate and Advanced – user-assigned

Service level access – factory-set

Electrical

Power supply ranges

100 to 240 V AC max., 50/60 Hz $\pm 10\%$

(90 to 264 V AC, 45/65 Hz)

Power consumption

<30 W

Terminal connections rating

AWG 26 to 16 (0.14 to 1.5 mm²)

Analog outputs

2 standard

2 optional

Galvanically isolated from the rest of the circuitry, 500 V for 1 minute. Range-programmable source and range 0 to 22 mA, max. load 750 W @ 20 mA

Relay outputs

4 standard

2 optional

Fully-programmable. Contacts rated at 2A @ 110/240 V Standard relays are changeover. Optional relays are normally closed (N/C).

Digital inputs / outputs

6 standard, user-programmable as input or output

Min. input pulse duration: 125 ms

Input:

volt-free or 24 V DC (conforms to IEC 61131-2)

Output:

open-collector, 30 V, 100 mA max.

(conforms to IEC 61131-2)

Connectivity/communications

Ethernet

PROFIBUS® DP

DP-V1

Modbus®

RTU, RS485, 2-wire/4-wire

Data logging

Storage

Measurement value storage (programmable sample rate)

Audit log*, Alarms log*, Calibration log, Diagnostics log,

Configuration changes

Chart view

On local display

Historical review

Of data

Data transfer

SD card interface/USB stick –

Windows®-compatible FAT file system, data and

log files in Microsoft® Excel® and DataManager Pro


-compatible formats

* Audit Log and Alarm Log data are stored in the same log file.

Overall dimensions


Transmitter

Dimensions in mm (in)

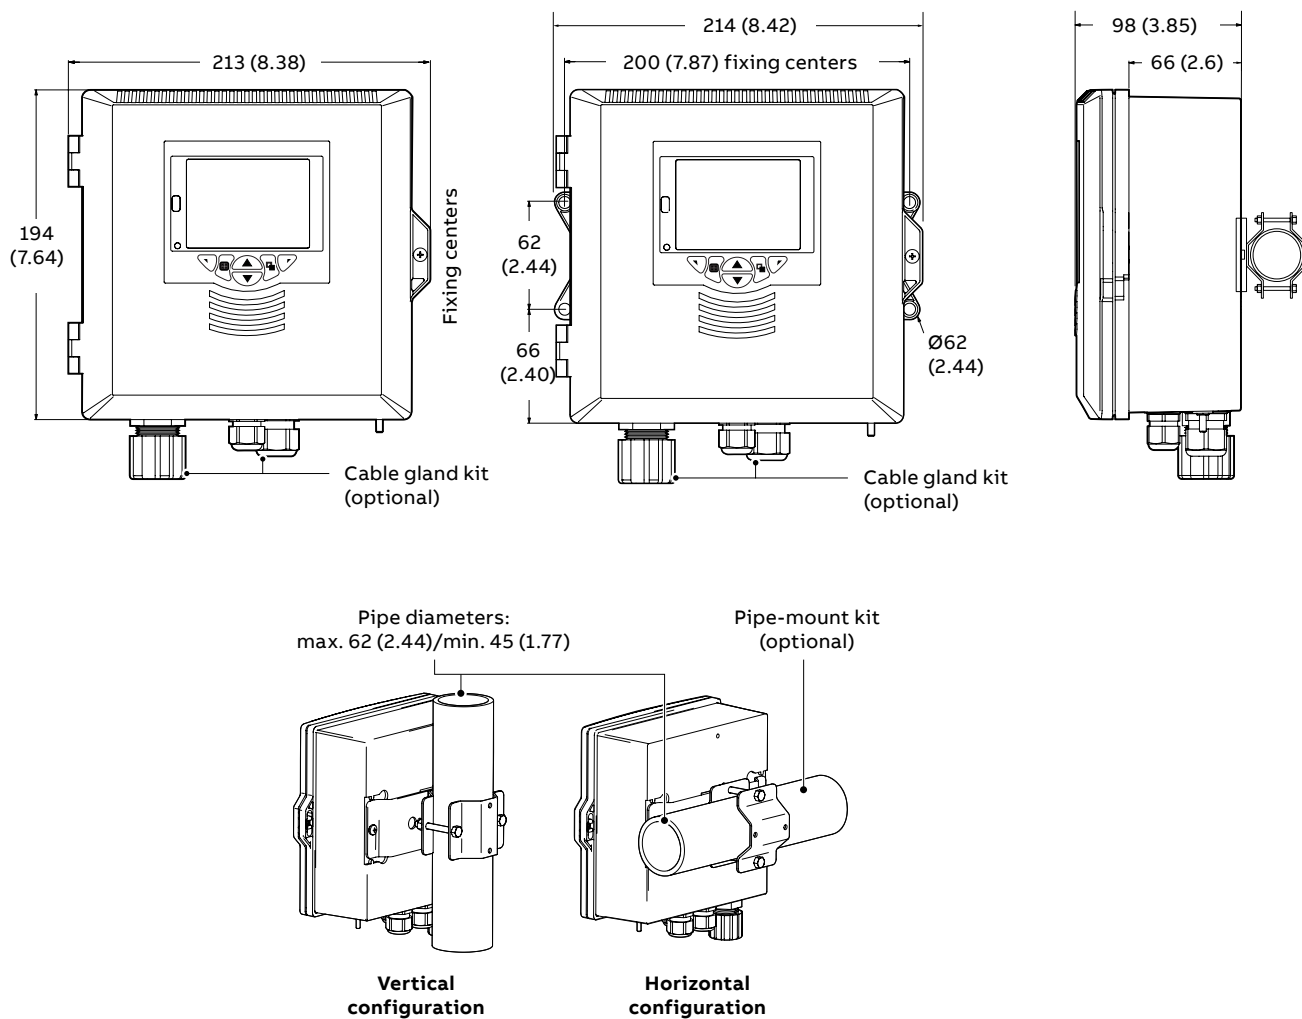


Wet section – ADS550

Dimensions in mm (in)

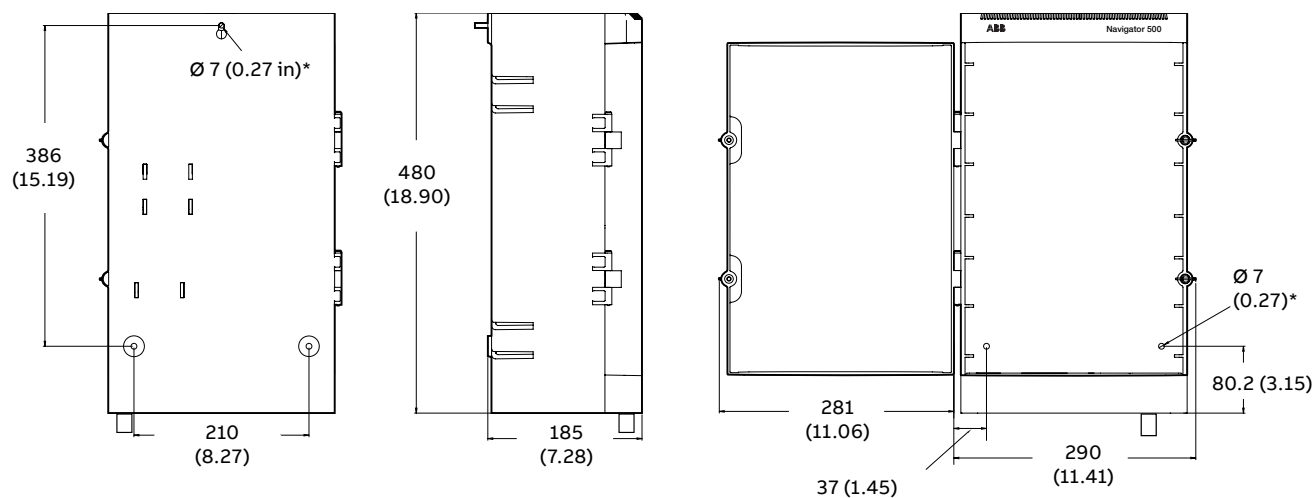
**Wet section – ADS551**







Dimensions in mm (in)

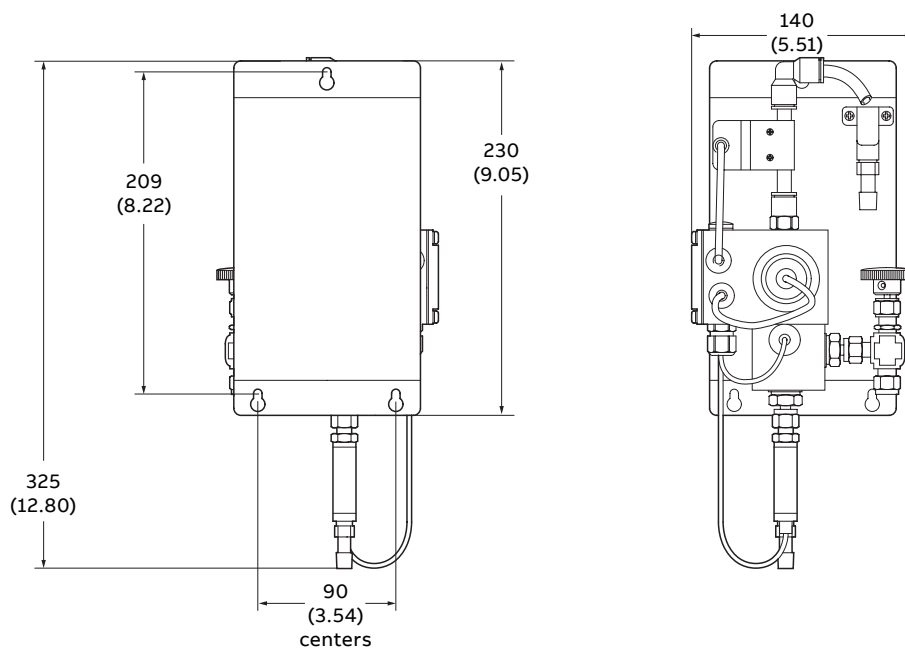


Electrical connections

Transmitter

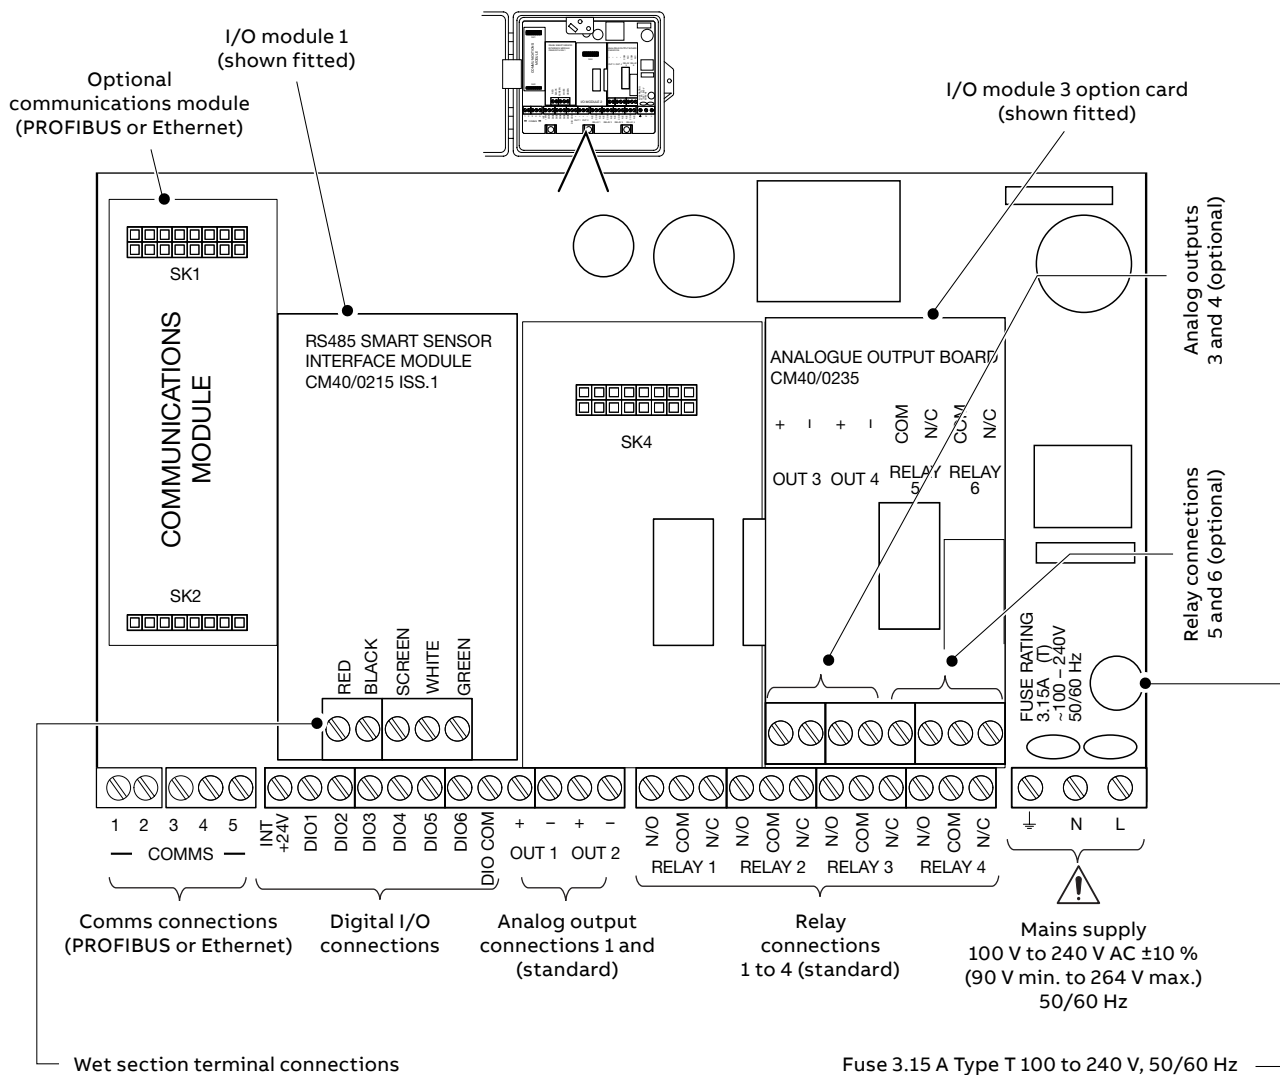


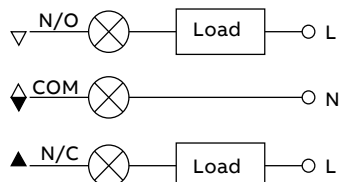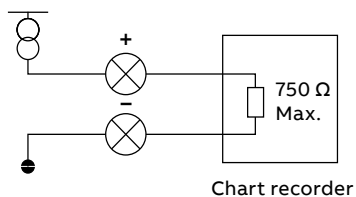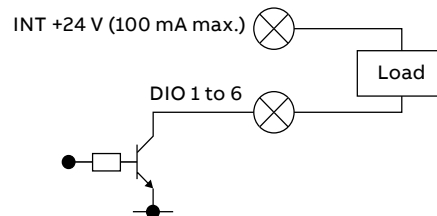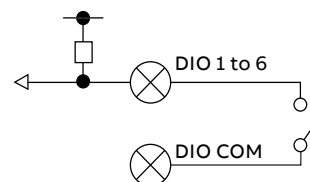Digital I/O, relays and analog output**Relays (1 to 4)****Analog outputs (1 to 4)****Relays (5 and 6)****Digital input (24 volt)****Digital output****Digital input (voltage-free)****Wet section – ADS550**

(applicable only to multiple wet section systems)

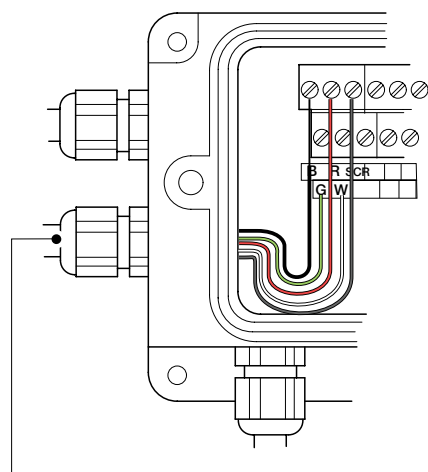**Additional serial cable connections to multiple wet sections**

Red – R (24 V)
 Black – B (0 V)
 Green – G (Data +ve)
 White – W (Data -ve)
 Screen – SCR

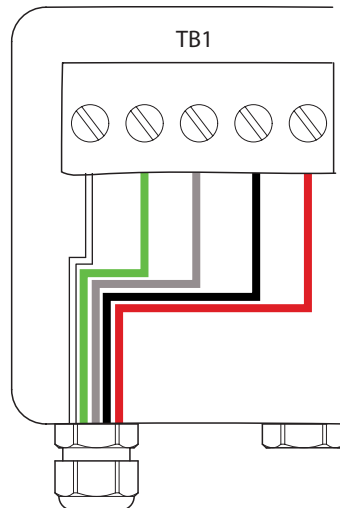Wet section – ADS551**Additional serial cable connections to multiple wet sections**

White – W (Data -ve)
 Green – G (Data +ve)
 Screen – SCR
 Black – B (0 V)
 Red – R (24 V)

Ordering information

Wet section – ADS550

Navigator 500 dissolved oxygen analyzer	ADS550/	X	X	X	X	XX	XX	Options
Build revision								
Reserved	A							
Measurement range								
Standard (0 to 20,000 ppb)		1						
Enclosure type								
Wall			W					
Number of streams								
Single stream				1				
Sensor type								
Standard						S1		
Supplied without sensor						Y0		
Process connection type								
6 mm fitting							A1	
¼ in fitting							B1	
Optional ordering codes								
Add 1 or more of the following codes after the standard ordering information to select any additional options.								
Sample measurement options								
Sample flow measurement								S1
Signal cable length and type (supplied without signal cable as standard)								
1.5 m (approx. 5 ft) cable, terminal connection								SC1
5 m (approx. 15 ft) cable, terminal connection								SC2
10 m (approx. 30 ft) cable, terminal connection								SC3
20 m (approx. 60 ft) cable, terminal connection								SC4
Test certificate								
Test certificate								CD
Documentation language* (supplied in English as standard)								
English								M5

* Commissioning instructions are supplied with each transmitter. Comprehensive operating instructions are available as a free download from www.abb.com or printed copies can be ordered as additional items.

Wet section – ADS551

Navigator 500 dissolved oxygen sensing system	ADS551/	X	X	X	X	XX	XX	Options
Build revision								
Reserved	A							
Measurement range								
Standard (0 to 20,000 ppb)		1						
Enclosure type								
Wall			W					
Number of streams								
Single stream				1				
Sensor type								
Standard						S1		
Supplied without sensor						Y0		
Process connection type								
6 mm fitting							A1	
1/4 in fitting							B1	

Optional ordering codes

Add 1 or more of the following codes after the standard ordering information to select any additional options.

Sample measurement options		
Auto calibration valve		A1
Sample flow control valve		B1
Sample flow measurement		S1
Signal cable length and type (supplied without signal cable as standard)		
1.5 m (approx. 5 ft) cable, terminal connection		SC1
5 m (approx. 15 ft) cable, terminal connection		SC2
10 m (approx. 30 ft) cable, terminal connection		SC3
20 m (approx. 60 ft) cable, terminal connection		SC4
Test certificate		
Test certificate		CD
Documentation language* (supplied in English as standard)		
English		M5

* Operating instructions are available as a free download from www.abb.com or printed copies can be ordered as additional items.

Ordering information

Transmitter

Navigator 540 transmitter	AWT540/	X	X	X	X	XX	XX	XX	XX	XX	Options
Build revision											
Reserved		A									
Enclosure type											
Wall mount			1								
Display type											
Color (standard)				A							
Power supply											
90 to 260 V AC, 50 to 60 Hz					1						
Channel 1											
Digital, wired sensor connection						B1					
Without						Y0					
Reserved							Y0				
Reserved								Y0			
Output signal											
Without									Y0		
Additional output card (2 current outputs + 2 relays)									Y2		
Ethernet									E1		
PROFIBUS DPV1									D1		
Data storage											
Without										Y0	
SD card function										D1	
USB function										D8	

Optional ordering codes

Add 1 or more of the following codes after the standard ordering information to select any additional options.

Accessories		
Panel mount kit		A2
Test certificate		
Test certificate		CD
Documentation language* (supplied in English as standard)		
English		M5
Cable entry options		
Metric gland pack (9 glands)		U1

* Commissioning instructions are supplied with each transmitter. Comprehensive operating instructions are available as a free download from www.abb.com or printed copies can be ordered as additional items.

Acknowledgements

- Excel is a registered trademark of Microsoft Corporation in the United States and/or other countries.
- Microsoft is a registered trademark of Microsoft Corporation in the United States and/or other countries.
- PROFIBUS is a registered trademark of PROFIBUS Nutzerorganisation, e.V.
- SD is a trademark of SD-3C.



Notes

Sales



Service



Software



ABB Measurement & Analytics

For your local ABB contact, visit:
abb.com/contacts

For more product information, visit:
abb.com/measurement








We reserve the right to make technical changes or modify the contents of this document without prior notice. With regard to purchase orders, the agreed particulars shall prevail. ABB does not accept any responsibility whatsoever for potential errors or possible lack of information in this document.

We reserve all rights in this document and in the subject matter and illustrations contained therein. Any reproduction, disclosure to third parties or utilization of its contents – in whole or in parts – is forbidden without prior written consent of ABB.

© Copyright 2024 ABB.
All rights reserved.



Our offering:

	Actuators and Positioners		Analytical Instruments
	Device Management, Fieldbus and Wireless		Flow Measurement
	Force Measurement		Level Measurement
	Natural Gas Measurement		Pressure Measurement
	Recorders and Controllers		Temperature Measurement

HMI – Automação e Instrumentação, Lda.

Travessa da Indústria, nº 111
4780-573 Santo Tirso
PORTUGAL

Tel. +351 252 850 501
Fax. +351 300 013 487

Web: www.hmi.pt

Email: hmi@hmi.pt